

Ova-Peptide Conjugation Kit (CM52418x1 and CM52418x3) User Reference Guide

Contents

Important Notes & Contact Information	2
Kit Components.....	3
Safety Information	3
Labeling Chemistry.....	3
Protocol.....	5
1. Lab Instrumentation Needed.....	5
2. Ova Conjugation with Peptide	5
3. Purification to Remove Excess Peptide.....	7
Other Considerations.....	9
1. Concentration Determination.....	9
2. MW Calculation.....	9
3. Recommended Storage Conditions	9
4. Peptide-to-Ova Ratio	9
5. Sample Submission for HPLC Analysis	9



CellMosaic, Inc.
10A Roessler Road
Woburn, MA 01801
USA

Phone: 781-463-0002
Fax: 781-998-4694
Email: info@cellmosaic.com
Website: www.cellmosaic.com

Important Notes & Contact Information

READ BEFORE USING ANY RESOURCES PROVIDED HEREIN

The information provided in this document and the methods included in this package are for information purposes only. CellMosaic provides no warranty of performance or suitability for the purpose described herein. The performance of labeling using this kit may be affected by many different variables, including but not limited to: purity and complexity of the peptide, differences in preparation techniques, operator abilities, and environmental conditions.

Sample data are provided for illustration and example purposes only and represent a small dataset used to verify kit performance in the CellMosaic laboratory. Information about the chemicals and reagents used in the kit are provided as necessary.

For Research Use Only. Not for Use in Diagnostic Procedures.

The information in this document is subject to change without notice. CellMosaic assumes no responsibility for any errors that may appear in this document. In no event shall CellMosaic be liable, whether in contract, tort, warranty, or under any statute or on any other basis for special, incidental, indirect, punitive, multiple, or consequential damages in connection with or arising from this document, including but not limited to the use thereof.


NOTICE TO PURCHASER: LIMITED LICENSE

The purchase of this product includes a limited, non-transferable license to use this product to practice the labeling methods using the reagents solely for the purchaser's research activities. The license granted herein is personal to the original purchaser and may not be transferred to any other party outside the purchaser's company. No other right or license is conveyed or granted either expressly, by implication or by estoppel, to resell or repackage this product. Further information can be obtained by contacting:

Director of Licensing
c/o CellMosaic, Inc.
10-A Roessler Road, Woburn, MA 01801
Phone: 781-463-0002
Fax: 781-998-4694
E-mail: info@cellmosaic.com

Kit Components

This kit provides materials to perform ovalbumin (Ova) labeling of one (CM52418x1) or three peptide samples (CM52418x3).

 Upon receipt, please remove **Box 1** and store in a freezer at or below -20°C . Store **Box 2** in a refrigerator at $2-8^{\circ}\text{C}$.

	Name	Part #	Quantity (CM52418x1)	Quantity (CM52418x3)	Storage condition
Box 1	Activated Ova (red label)	CM52114	1x2 mg	3x2 mg	-20°C
Box 2	Solution A (green label)	CM01003	1.5 mL	3 mL	$2-8^{\circ}\text{C}$
	Solution B (purple label)	CM01007	0.5 mL	0.5 mL	
	1xPBS buffer	CM02013	6 mL	20 mL	
	Centrifuge filter device s	CM03CD030A	2	6	
	Collection tubes	CM03CT0	4	12	
	1.5 mL centrifuge tube(s)	CM03CT2	1	3	
	0.5 mL centrifuge tube(s)	CM03CT1	1	3	
User Material	Cys-peptide	N/A	NOT PROVIDED (User Supplied Material. 0.23–0.9 μmol for each reaction)		

Cys-peptide amount: This kit uses Ova modified with a high number of maleimide groups (10–20 average maleimides per Ova, please check the COA of each individual batch for the exact number of maleimide per Ova. **Note:** you cannot achieve loading greater than the number of maleimides). 0.23–0.9 μmole peptide will correspond to 5–20 equivalents of peptide over Ova.

Peptide to Ova ratio optimization: Peptide loading will be determined primarily by the amount of peptide added during the labeling if the equivalents of peptide over Ova is less than the maleimide groups per Ova. By balancing the amount of activated Ova and peptide added, the loading can be optimized to your target value (See Note in **Step A4**). You can experimentally measure the peptide loading by checking the % of peptide consumed during the labeling reaction (See HPLC or UV sampling and calculation in **Step A3** and **B6**).

Safety Information

Warning: some of the chemicals used can be potentially hazardous and can cause injury or illness. Please read and understand the Material Safety Data Sheets (MSDS) available at CellMosaic.com before you store, handle, or use any of the materials.

Labeling Chemistry


Ovalbumin (Ova) is a small protein sometimes used as a carrier protein for antibody production. Chicken egg albumin is the major protein constituent of egg whites and has a MW of 44.3 KDa if the carbohydrate and phosphate portions are accounted. CellMosaic has designed this personalized Ova

conjugation kit to work with any peptide containing a reactive Cys group. The user supplies their own peptide. Using the kit components, the customer prepares the Ova-peptide conjugate by reacting the peptide (customer supplied) with activated Ova. One-step purification typically provides the resulting Ova-peptide at greater than 95% purity.

This kit provides materials to perform Ova labeling of one to three peptides. The total amount of activated Ova included in a reaction: 2 mg.

Key features of this Ova-peptide conjugation kit:

- High quality maleimide-activated Ova for the conjugation: >99% purity
- High maleimide groups per Ova for peptide loading: 10–20 (please check the COA of each individual batch for the exact loading)
- A single purification affords over 95% of the Ova-peptide conjugates
- Fast preparation: less than 1 h hands-on time
- All reagents and consumables are included, from preparation to purification
- Options to choose tailored custom services at CellMosaic prior to and after conjugation in your lab:
 - Prior to conjugation, you can supply your peptide information when you place your order and CellMosaic will give recommendations for the conjugation if your peptide has special features (complementary service);
 - After conjugation you can choose to send your sample to CellMosaic for HPLC analysis of the conjugate or peptide samples for determination of the peptide loading.

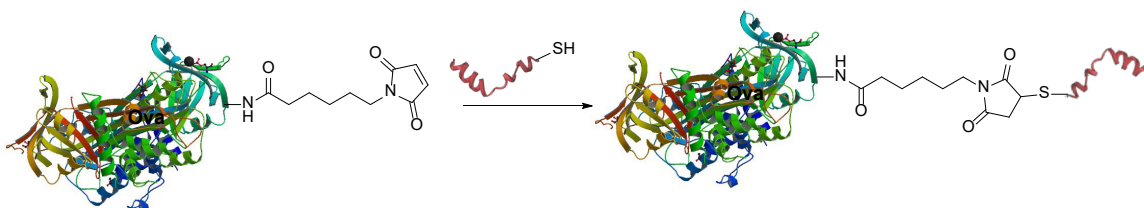


Requirement for Cys-peptide:

1. Amount: 0.23–0.9 μmol (5–20 equivalents of peptide over Ova)
2. HPLC purified and lyophilized: please ensure no reducing reagents, such as DTT, are present
3. The Cys-peptide should be stored at -80°C
4. HPLC purity: >85% for *N*-terminal Cys peptide and >90% for *C*-terminal Cys peptide

Potential interfering compounds for labeling and conjugation reactions:

Thiols: e.g., DTT and mercaptoethanol

Protocol

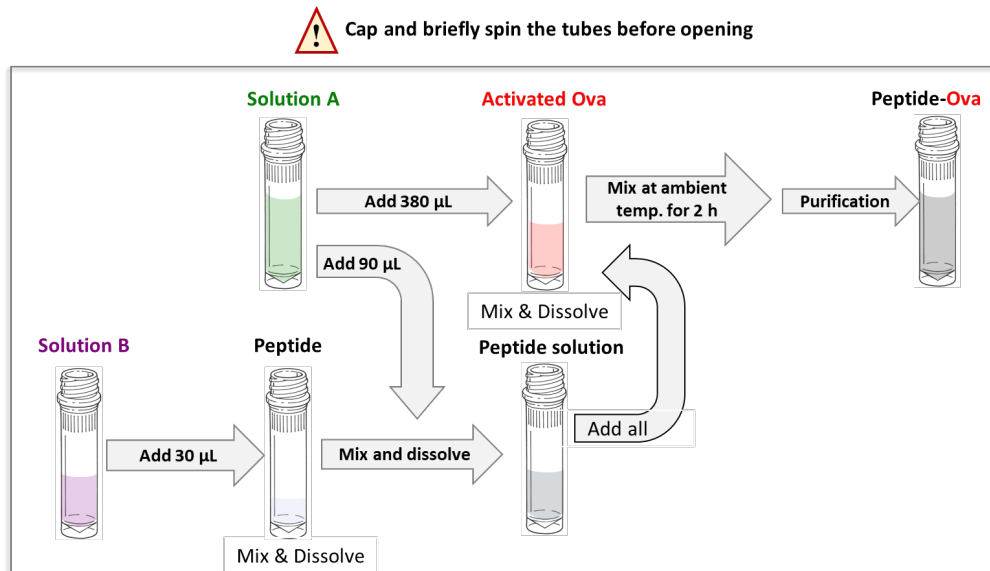

Scheme 1. Schematic diagram of the workflow for preparing peptide-Ova conjugates.

1. Lab Instrumentation Needed

- Vortex mixer, centrifuge (preferably refrigerated)
- Pipettes and tips
- Timer
- Incubator or shaker set at 25°C or RT
- Balance

2. Ova Conjugation with Peptide

A1. Add 380 µL of **Solution A** (green label) to a tube containing **Activated Ova** (red label). Vortex for 30 seconds to 1 minute to dissolve the Ova.



The following steps (**A2**, **A3**, and **A4**) are to be performed without any break. Cys peptide, once dissolved in solution, tend to oxidize quickly, and should be used immediately. Do not store any Cys peptide solution for later usage.

A2. Weigh 0.23-0.9 µmol of **Cys-peptide** quickly into a 0.5 mL microcentrifuge tube. **Note:** the peptide in general is static charged. Use the tip of a glass Pasteur pipet to weigh the peptide if possible. It may be difficult to obtain the exact weight. Any amount between 0.23-0.9 µmol is acceptable (no need to adjust the volume of the dissolving solution).

Calculation for 0.23 µmol (target 5 peptides per Ova if all the peptides are labeled):

Amount of Cys-peptide (mg) = Molecular weight of Cys-peptide x 0.00023

Calculation for 0.9 μmol (target 15-20 peptides per Ova):

Amount of Cys-peptide (mg) = Molecular weight of Cys-peptide x 0.0009

A3. Add 30 μL of **Solution B** (purple label) to the centrifuge tube containing Cys-peptide from **Step A2**. Vortex for 30 seconds and centrifuge the tube to get all of the liquid down to the bottom. Open the cap and add 90 μL of **Solution A** (green label) to the tube. Vortex for 30 seconds or sonicate for a few minutes to ensure all of the solid is dissolved. Discard any unused **Solution B** as hazardous chemical waste **until the experiments are done**.

Tip for solubility check (Step A3): It may take a while for your peptide to fully dissolve. In general, most of the peptide should be able to dissolve in this mixed solution system. Check the bottom of the micro-centrifuge tube to ensure the solution is clear and free of any solid residue. If some solid remains after a few minutes, centrifuge the tube and pipette the supernatant for the next step.

Tip for opening centrifuge tube after vortex: Always centrifuge the tube to ensure no liquid is in the cap.

HPLC or UV Sample (A3) for peptide loading measurement (Optional): If you are planning to experimentally determine the peptide loading, please follow the steps below:

- Transfer 6 μL of the peptide solution from **Step A3** (5% of the total amount) to a new centrifuge tube and label it as **sample A3**.
- For UV measurement, dilute the sample 10-50 times in 50% MeOH/water. Record the dilution factor DF(A3) and UV absorbance at 280 nm (A(A3)). Remember to use 50% MeOH/water as a blank for subtraction.
- For HPLC analysis, dilute the sample 5-20 times in 50% MeOH/water (detect at 205 and 280 nm). Record the dilution factor DF(A3) and HPLC Area (A(A3)).

A4. Transfer the solution from **Step A3** to the tube containing **Activated Ova** from **Step A1**. Pipette the solution up and down in the tube three times to mix. Incubate at room temperature for 2 hours (**Note:** if you use the decreased amount of **Activated Ova**, please pipette out the desired volume of **Activated Ova** from **Step A1** to the peptide solution from **Step A3** instead).

Peptide Loading Optimization: The desired peptide loading is specific to the project. Recommended target peptide loading is within 5–20 peptides per Ova. Your target loading can be adjusted by either changing the moles of peptide added in **Step A2** or the volume of activated Ova from **Step A1**. You can also change both.

Calculation of the theoretical loading if 100% peptide are labeled:

$$\text{Peptide per Ova (Loading)} = \frac{P \times V(A4) \times 8417}{O \times 120}$$

V(A4): total volume of peptide added in **Step A4** (μL)

P: total amount of peptide added in **Step A2** (μmol)

O: total volume of activated Ova added in **Step A4** (μL)

3. Purification to Remove Excess Peptide

B1. Place the centrifuge tube from **Step A4** containing the reaction mixture into the centrifuge rotor and counterbalance with a similar device. Spin **the centrifuge tube** at 10,000 x g for 2 minutes.

B2. Insert the **Filter Device** into one of the provided collection tubes (micro-centrifuge tube with the cap attached). Transfer and divide the supernatant from **Step B1** into two **Centrifuge Filter Devices**. Add 250 µL of **PBS Buffer** to make up the total volume to 500 µL in each filter device and cap it.

B3. Place the assembled **Filter Devices** into the centrifuge rotor, aligning the cap straps toward the center of the rotor. Spin the assembled **Filter Devices** at 14,000 x g for 8 minutes to concentrate down to < 100 µL (Spin time depends on many factors. A typical spin time for a 500 µL sample is approximately 8 to 20 minutes. The typical volume is ~40 µL of residual fluid in each filter device after spinning for 8 minutes on an Eppendorf 5417R at 4°C).

B4. Remove the assembled devices from the centrifuge and separate the **Filter Device** from the collection tube. Transfer the filtrate from the collection tubes to a clean centrifuge tube (not provided). **Save the filtrate for UV or HPLC analysis.**

B5. Insert the **Filter Device** back into the collection tube. Add 400 µL of **PBS Buffer** to make up the total volume to 500 µL in each filter device and cap it. Place the two assembled **Filter Devices** into the centrifuge rotor, aligning the cap strap toward the center of the rotor. Spin the assembled **Filter Devices** at 14,000 x g for 8 minutes.

B6. If the MW of your peptide is <3000 Da, repeat **Step B5** two times.

If the MW of your peptide is between 3000-5000 Da, repeat **Step B5** three times.

If the MW of your peptide is >5000 Da, repeat **Step B5** four times.

HPLC or UV Sample (B6) for peptide loading measurement (Optional): If you are planning to experimentally determine the peptide loading, please follow these steps:

- Combine the first three purification filtrates from **Steps B4–B6** and label it as **sample B6**. Record the total volume of the filtrate (~2.4 mL).
- For UV measurement, record the absorbance of the sample at 280 nm without dilution (A(B6)). Remember to use PBS buffer as a blank for subtraction
- For HPLC analysis, inject the sample without dilution and detect the peak at 205 and 280 nm. Record the HPLC area (A(B6)).

Calculation of the peptide to Ova ratio:

$$\text{Peptide per Ova} = \frac{P}{O} \times \frac{V(A4)}{120} \times \left(1 - \frac{A(B6) \times V(B6)}{A(A3) \times DF(A3) \times V(A4)} \right) \times 8417$$

A(A3): UV absorbance at 280 nm or HPLC area of sample A3 (blank subtracted)

A(B6): UV absorbance at 280 nm or HPLC area of sample B6 (blank subtracted)

DF(A3): dilution factor of sample A3

V(B6): total volume of filtrate B6 (μL)
V(A4): total volume of peptide added **Step A4** (μL)
P: total amount of peptide added in **Step A2** (μmole)
O: total volume of activated Ova added in **Step A4** (μL)

B7. To recover the conjugates, place the **Filter Device** upside down in a clean **Collection Tube**. Place in the centrifuge, aligning the open cap towards the center of the rotor. Spin for 2 minutes at 1,000 x g to transfer the conjugates from the **Filter Devices** to the **Collection Tubes**.

B8. Transfer the conjugates from the two **Collection Tubes** to a 1.5 mL micro-centrifuge tube.

B9. Rinse each **Collection Tube** with 50 μL of **PBS Buffer** and transfer the entire contents to the 1.5 mL micro-centrifuge tube from **Step B8**.

B10. Add 100 μL of **PBS Buffer** to each **Filter Device** to rinse. Stir it gently with a pipet tip, then transfer the entire contents to the 1.5 mL micro-centrifuge tube from **Step B8**. Add **PBS Buffer** to make the total volume of the sample 400 μL and cap it (use the pipetman to measure the total volume).

B11. Vortex the combined protein sample for 30 seconds and then centrifuge to ensure no liquid is in the cap.

Ova-Peptide is Ready for Your Experiment

Tip: The approximate concentration of the **Ova-peptide conjugate** is 90 μM in 400 μL of PBS buffer (assuming 80% recovery). You can also determine the concentration using a UV/Vis spectrophotometer. For downstream applications, avoid using any buffer that contains free thiol (e.g., Cys).

Other Considerations

1. Concentration Determination

To determine the concentration, dilute your Ova-peptide from **Step B11** with 1x PBS buffer. Measure the UV absorbance of the Ova-peptide at 280 nm (A_{280}) using a UV spectrometer and calculate the concentration using the following formula:

$$\text{Concentration } (\mu\text{M}) \text{ of the dilute sample} = (A_{280}) / (L \times \epsilon)$$

Where A_{280} is the absorbance of Ova-peptide conjugates at 280 nm; L is the UV cell path length (cm); and ϵ is the extinction coefficient of the Ova-peptide conjugate at 280 nm.

If you know the sequence of the peptide and the average molar ratio of peptide per Ova, you can calculate ϵ as described in the following equation (Gill, S.C. and von Hippel, P. H. *Anal. Biochem.* **1989**, *182*, 319–326; Pace, C.N., *et al. Protein Sci.* **1995**, *4*, 2411–2423):

$$\epsilon = m \times ((nW \times 5500) + (nY \times 1490) + (nC \times 125)) + 30590$$

Where m is the average molar ratio of peptide per Ova. If you do not know the molar ratio, you can use the amount of peptide added.

Where n is the number of corresponding residues present in the peptide: tryptophan (W), tyrosine (Y), and cysteine (C).

If you are using a 1 cm UV cell, you can dilute the Ova-peptide 10-20 times to get a good reading.

2. MW Calculation

Calculation of the MW of the conjugate:

$$\text{MW(conjugate)} = m \times \text{MW(peptide)} + 44300$$

Where m is the average molar ratio of peptide per Ova.

3. Recommended Storage Conditions

For long-term storage, Ova-peptide conjugates can be stored frozen at -20°C.

4. Peptide-to-Ova Ratio

Peptide loading can be measured experimentally by checking the % of peptide consumed during the labeling reaction. Please see HPLC or UV sampling and calculation of peptide-to-Ova ratio in **Step A3** and **B6**.

5. Sample Submission for HPLC Analysis

If you are submitting samples to CellMosaic for C18 HPLC analysis for sample loading and SEC HPLC for conjugate analysis, please follow these instructions:

- 1) Go online: <https://www.cellmosaic.com/hplc-analysis/>, select C18 HPLC Analysis ([Product# AS0021](#)) and SEC HPLC Analysis ([Product# AS0023](#)), choose the quantity (number of samples - bulk discounts are available for multiple samples), and submit the order. Alternatively, you can email info@cellmosaic.com for a quote and to place the order.
- 2) For peptide loading determination by C18 HPLC, transfer sample **A3** and **B6** to a micro-centrifuge tube with screw cap and label the vial properly.
- 3) For conjugate purity analysis by SEC HPLC, mix 10 μ L of your conjugate from **Step B11** with 40 μ L of 1x PBS buffer into a micro-centrifuge tube with screw cap. Label the vial properly.
- 4) Ship your samples with a cold pack for overnight or 2nd day delivery.